

## Human PECAM1 / CD31 ELISA Kit

Catalog No. CDK013B

Quantity: 2 x 96 tests

### PRODUCT SPECIFICATIONS :

**Specificity :** Recognizes both natural and recombinant human soluble PECAM-1

**Range :** 0.31 ng/ml - 10 ng/ml

**Sensitivity :** <0.17 ng/ml

**Incubation :** 2 hours, 45 min

**Sample Types :** Serum  
Plasma  
Cell culture supernatant

**Cross Reaction :** No cross reactivity with other human adhesion molecules

**Kit Content :** Pre-coated 12 strip plates, biotinylated secondary antibody, standards, controls, buffers, Streptavidin-HRP, TMB, Stop Reagent.

### 1. INTENDED USE

The Cell Sciences<sup>®</sup> Human CD31 (PECAM-1) ELISA is to be used for the *in-vitro* qualitative and quantitative determination of CD31 (PECAM-1) in cell culture supernatants, buffered solutions or human serum and plasma samples. This assay will recognize natural human CD31. **This kit has been configured for research use only.**

### 2. PRINCIPLE OF THE METHOD

A monoclonal capture antibody highly specific for CD31 has been coated to the wells of the microtiter strip plate provided during manufacture. Binding of CD31 samples and known standards to the capture antibodies and subsequent binding of the biotinylated anti-CD31 secondary antibody to the analyte is completed during the same incubation period. Any excess unbound analyte and secondary antibody is removed.

The HRP conjugate solution is then added to every well including the zero wells, following incubation excess conjugate is removed by careful washing.

A chromogen substrate is added to the wells resulting in the progressive development of a blue colored complex with the conjugate. The color development is then stopped by the addition of acid turning the resultant final product yellow. The intensity of the produced colored complex is directly proportional to the concentration of CD31 present in the samples and standards.



**Cell Sciences, Inc.<sup>®</sup>**  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888-769-1246  
Phone: 978-572-1070  
Fax: 978-992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)

The absorbance of the color complex is then measured and the generated OD values for each standard are plotted against expected concentration forming a standard curve. This standard curve can then be used to accurately determine the concentration of CD31 in any sample tested.

### 3. REAGENTS PROVIDED AND RECONSTITUTION

Reagents (Store @ 2-8°C)	Quantity 2 x 96 well kit	Reconstitution
P: 96 well microtiter strip plate	2	Ready to use. (Pre-coated)
A: Plastic plate covers	4	n/a
B: Standard: 10 ng/ml	4 vials	Reconstitute as directed on the vial. (see Assay preparation, section 8)
C: Standard Diluent (Buffer)	1 vial (25 ml)	10x Concentrate, dilute in distilled water (see reagent preparation, section 8).
D: CD31 Control	4 vials	Reconstitute as directed on the vial (see reagent preparation, section 8)
E: Biotinylated anti-CD31	2 vials ( 0.4 ml)	Dilute in biotinylated antibody diluent (see reagent preparation, section 8).
F: Biotinylated Antibody diluent	1 vial (13 ml)	Ready to use.
G: Streptavidin-HRP	4 vials (5 µl)	Add 0.5 ml of HRP diluent prior to use. (see Assay preparation, section 8)
H: HRP Diluent	1 vial (23 ml)	Ready to use.
I: Wash Buffer	2 vials (10 ml)	200x Concentrate, dilute in distilled water. (see Assay preparation, section 8)
J: TMB Substrate	1 vial (24 ml)	Ready to use.
K: H <sub>2</sub> SO <sub>4</sub> stop reagent	2 vial (11 ml)	Ready to use.

### 4. MATERIAL REQUIRED BUT NOT PROVIDED

- Microtiter plate reader fitted with appropriate filters (450 nm required with optional 620 nm reference filter)
- Microplate washer or wash bottle
- 10, 50, 100, 200 and 1,000 µl adjustable single channel micropipettes with disposable tips
- 50-300 µl multi-channel micropipette with disposable tips
- Multichannel micropipette reagent reservoirs
- Distilled water
- Vortex mixer
- Miscellaneous laboratory plastic and/or glass, if possible sterile



## 5. STORAGE INSTRUCTIONS

Store the kit reagents between 2 and 8 °C. Immediately after use, remaining reagents should be returned to cold storage (2-8 °C). The expiration date of the kit and reagents is stated on box front labels. The expiration of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, the reagent is not contaminated by the first handling.

**Wash Buffer 1X:** Once prepared, store at 2-8 °C for up to 1 week.

**Standard Diluent Buffer 1X:** Once prepared, store at 2-8 °C for up to 1 week.

**Reconstituted Standards/Controls:** Once prepared, use immediately and do not store.

**Diluted Biotinylated Secondary Antibody:** Once prepared, use immediately and do not store.

**Diluted Streptavidin-HRP:** Once prepared, use immediately and do not store.

## 6. SPECIMEN COLLECTION, PROCESSING & STORAGE

Cell culture supernatants, serum, plasma or other biological samples are suitable for use in the assay. Remove serum from the clot or red cells respectively, as soon as possible after clotting and separation.

**Cell culture supernatants:** Remove particulates and aggregates by spinning at approximately 1000 x g for 10 min.

**Serum:** Use pyrogen/endotoxin free collecting tubes. Serum should be removed rapidly and carefully from the red cells after clotting. Following clotting, centrifuge at approximately 1000 x g for 10 min and remove serum.

**Plasma:** EDTA, citrate and heparin plasma can be assayed. Spin samples at 1000 x g for 30 min to remove particulates. Harvest plasma.

**Storage:** If not analyzed shortly after collection, samples should be aliquoted (250-500 µl) to avoid repeated freeze-thaw cycles and stored frozen at -70 °C. Avoid multiple freeze-thaw cycles of frozen specimens.

**Recommendation:** Do not thaw by heating at 37 °C or 56 °C. Thaw at room temperature, and make sure that the sample is completely thawed and homogeneous before use. When possible, avoid use of badly hemolyzed or lipemic sera. If large amounts of particles are present, these should be removed prior to use by centrifugation or filtration.

## 7. SAFETY AND PRECAUTIONS FOR USE

- Handling of reagents, serum, or plasma specimens should be in accordance with local safety procedures, e.g. CDC/NIH Health manual: "Biosafety in Microbiological and Biomedical Laboratories" 1984.



Cell Sciences, Inc.<sup>®</sup>  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888-769-1246  
Phone: 978-572-1070  
Fax: 978-992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)

- Laboratory gloves should be worn at all times.
- Avoid any skin contact with H<sub>2</sub>SO<sub>4</sub> and TMB. In case of contact, wash thoroughly with water.
- Do not eat, drink, smoke or apply cosmetics where kit reagents are used.
- Do not pipette by mouth.
- When not in use, kit components should be stored refrigerated or frozen, as indicated on vial or bottle labels.
- All reagents should be warmed to room temperature before use. Lyophilized standards should be discarded after use.
- Once the desired number of strips has been removed, immediately reseal the bag to protect the remaining strips from deterioration.
- Cover or cap all reagents when not in use.
- Do not mix or interchange reagents between different lots.
- Do not use reagents beyond the expiration date of the kit.
- Use a clean, disposable, plastic pipette tip for each reagent, standard, or specimen addition in order to avoid cross contamination for the dispensing of H<sub>2</sub>SO<sub>4</sub> and substrate solution. Avoid pipettes with metal parts.
- Use a clean plastic container to prepare the washing solution.
- Thoroughly mix the reagents and samples before use by agitation or swirling.
- All residual washing liquid must be drained from the wells by efficient aspiration, or by decantation, followed by tapping the plate forcefully on absorbent paper. Never insert absorbent paper directly into the wells.
- The TMB solution is light sensitive. Avoid prolonged exposure to light. Also, avoid contact of the TMB solution with metal to prevent color development. **Warning: TMB is toxic. Avoid direct contact with hands. Dispose of properly.**
- If a dark blue color develops within a few minutes after preparation, this indicates that the TMB solution has been contaminated and must be discarded. Read absorbances within 1 hour after completion of the assay.
- When pipetting reagents, maintain a consistent order of addition from well-to-well. This will ensure equal incubation times for all wells.
- Follow incubation times described in the assay procedure.
- Dispense the TMB solution immediately after washing of the microtiter plate.

## 8. ASSAY PREPARATION

Bring all reagents to room temperature before use.

### 8.1 Assay Design

Determine the number of microwell strips required to test the desired number of samples, plus appropriate number of wells needed for running zeros and standards. Each sample, standard and zero should be tested **in duplicate**. Remove sufficient Microwell Strips for testing from the pouch immediately prior to use. Return any wells not required for this assay with desiccant to the pouch. Seal tightly and return to 2-8 °C storage.



**Cell Sciences, Inc.**<sup>®</sup>  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888-769-1246  
Phone: 978-572-1070  
Fax: 978-992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)

**Example plate layout** (example shown for a 6 point standard curve)

	Standards / Controls		Sample Wells									
	1	2	3	4	5	6	7	8	9	10	11	12
A	10	10										
B	5	5										
C	2.5	2.5										
D	1.25	1.25										
E	0.63	0.63										
F	0.31	0.31										
G	zero	zero										
H	Ctrl	Ctrl										

*All remaining empty wells can be used to test samples in duplicate*

## 8.2 Preparation of Wash Buffer

Dilute the (200x) wash buffer concentrate 200 fold with distilled water to give a 1x working solution. Pour entire contents (10 ml) of the Washing Buffer Concentrate into a clean 2,000 ml graduated cylinder. Bring final volume to 2,000 ml with glass-distilled or deionized water. Mix gently to avoid foaming. Transfer to a clean wash bottle and store at 2°-8°C for up to 1 week.

## 8.3 Preparation of Standard Diluent Buffer

Add the contents of the vial (10x concentrate) to 225 ml of distilled water before use.

This solution can be stored at 2-8°C for up to 1 week.

## 8.4 Preparation of Standard

Standard vials must be reconstituted with the volume of standard diluent shown on the vial immediately prior to use. This reconstitution gives a stock solution of 10 ng/ml of CD31. Mix the reconstituted standard gently by inversion only. Serial dilutions of the standard are made directly in the assay plate to provide the concentration range from 10 to 0.31 ng/ml. A fresh standard curve should be produced for each new assay.

- Immediately after reconstitution add 200 µl of the reconstituted standard to wells A1 and A2, which provides the highest concentration standard at 10 ng/ml.
- Add 100 µl of Standard Diluent to the remaining standard wells B1 and B2 to F1 and F2
- Transfer 100 µl from wells A1 and A2 to B1 and B2. Mix the well contents by repeated aspirations and ejections taking care not to scratch the inner surface of the wells
- Continue this 1:1 dilution using 100 µl from wells B1 and B2 through to wells F1 and F2 providing a serial diluted standard curve ranging from 10 ng/ml to 0.31 ng/ml
- Discard 100 µl from the final wells of the standard curve (F1 and F2)



- Alternatively these dilutions can be performed in separate clean tubes and immediately transferred directly into the relevant wells.

## 8.5 Preparation of Controls

The supplied Controls must be reconstituted with the volume of Standard Diluent indicated on the vial. Reconstitution of the freeze-dried material with the indicated volume, will give a solution at the concentration stated on the vial. Allow to stand for 5 min with intermittent gentle swirling before use. Do not store after use.

## 8.6. Preparation of Samples

Before testing, serum or plasma samples have to be diluted 1:4 in standard diluent (buffer).

## 8.7. Preparation of Biotinylated anti CD31

It is recommended this reagent is prepared immediately before use. Dilute the biotinylated anti-CD31 with the biotinylated antibody diluent in an appropriate clean glass vial using volumes appropriate to the number of required wells. Please see example volumes below:

Number of wells required	Biotinylated Antibody ( $\mu$ l)	Biotinylated Antibody Diluent ( $\mu$ l)
16	40	1060
24	60	1590
32	80	2120
48	120	3180
96	240	6360

## 8.8 Preparation of Streptavidin-HRP

It is recommended to centrifuge vial for a few seconds in a microcentrifuge to collect all the volume at the bottom.

Dilute the 5  $\mu$ l vial with 0.5 ml of HRP diluent **immediately before use**. Do-not keep this diluted vial for future experiments. Further dilute the HRP solution to volumes appropriate for the number of required wells in a clean glass vial. Please see example volumes below:

Number of wells required	Streptavidin-HRP ( $\mu$ l)	Streptavidin-HRP Diluent (ml)
16	30	2
24	45	3
32	60	4
48	75	5
96	150	10



## 9. METHOD

We strongly recommend that every vial is mixed thoroughly without foaming prior to use.

Prepare all reagents as shown in section 8. Note: Final preparation of Biotinylated anti-CD31 (section 8.7) and Streptavidin-HRP (section 8.8) should occur immediately before use.

Assay Step		Details
1.	Preparation	<b>Prepare Standard Curve</b> as shown in 8.4
2.	Addition	Add 100 µl of each <b>standard, sample, control and zero</b> (Standard Diluent) in duplicate to appropriate number of wells
3.	Addition	Add 50µl of diluted <b>biotinylated anti-CD31</b> to all wells
4.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25 °C) for <b>1 hour</b> .
5.	Wash	Remove the cover and wash the plate as follows: a) Aspirate the liquid from each well. b) Dispense 0.3 ml of <b>1x washing solution</b> into each well. c) Aspirate the contents of each well. d) Repeat step b and c another two times.
6.	Addition	Add 100 µl of <b>Streptavidin-HRP</b> into all wells.
7.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25 °C) for <b>30 minutes</b> .
8.	Wash	Repeat wash as in Step 5.
9.	Addition	Add 100 µl of ready-to-use <b>TMB Substrate Solution</b> into all wells.
10.	Incubation	Incubate in the dark for <b>10-20 minutes*</b> at room temperature. Avoid direct exposure to light by wrapping the plate in aluminum foil.
11.	Addition	Add 100 µl of <b>H<sub>2</sub>SO<sub>4</sub>: Stop Reagent</b> into all wells.

**Read the absorbance** value of each well (immediately after step 11) on a spectrophotometer, using 450 nm as the primary wavelength, and optionally 630 nm as the reference wave length (610 nm to 650 nm is acceptable).

*\*Incubation time of the substrate solution is usually determined by the ELISA reader performance. Many ELISA readers only record absorbance up to 2.0 O.D. Therefore the color development within individual microwells must be observed by the analyst, and the substrate reaction stopped before positive wells are no longer within recordable range.*



## 10. DATA ANALYSIS


Calculate the average absorbance values for each set of duplicate standards and samples. Ideally, duplicates should be within 20% of the mean.

Generate a linear standard curve by plotting the average absorbance of each standard on the vertical axis versus the corresponding Human CD31 standard concentration on the horizontal axis.

The amount of CD31 in each sample is determined by extrapolating O.D. values against CD31 standard concentrations using the standard curve.

### Sample CD31 Standard Curve

Standard	CD31 Conc	OD (450nm) mean	CV (%)
1	10	2.101	1.82
2	5	1.260	0.11
3	2.5	0.766	10.62
4	1.25	0.503	3.94
5	0.63	0.268	5.80
6	0.31	0.160	11.49
zero	0	0.021	13.47

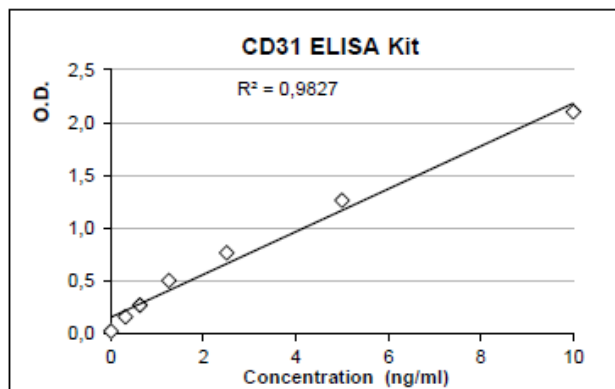

**Note:** The curve shown above should not be used to determine results. Every lab must produce a standard curve for each set of microwell strips assayed.

For serum or plasma samples which have been diluted 1:4 according to the protocol, the calculated concentration should be multiplied by the dilution factor (x4).

## 11. ASSAY LIMITATIONS

Do not extrapolate the standard curve beyond the maximum standard curve point. The dose-response is non-linear in this region and good accuracy is difficult to obtain. Concentrated samples above the maximum standard concentration must be diluted with Standard diluent or with your own sample buffer to produce an OD value within the range of the standard curve. Following analysis of such samples always multiply results by the appropriate dilution factor to produce actual final concentration.

The influence of various drugs on end results has not been investigated. Bacterial or fungal contamination and laboratory cross-contamination may also cause irregular results.

Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing fresh Washing Buffer, fill with Washing Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.

Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.

As with most biological assays conditions may vary from assay to assay therefore **a fresh standard curve must be prepared and run for every assay.**

## 12. PERFORMANCE CHARACTERISTICS

### 12.1 Sensitivity

The sensitivity or minimum detectable dose of human CD31 using this ELISA kit was found to be **0.04 ng/ml**. This was determined by adding 3 standard deviations to the mean OD obtained when the zero standard was assayed 40 times.

### 12.2. Specificity

The assay recognizes natural CD31.

To define the specificity of this ELISA several proteins were tested for cross reactivity. There was no cross reactivity observed for any protein tested (IL-2R/CD25, IL-4R/CD124, IL-6R/CD126, CD62P, Fas/CD95, CD117, CD141, TRAIL/CD253, TRAIL R1/CD261, gp130/CD130).

### 12.3. Precision

#### Intra-assay

Reproducibility within the assay was evaluated in three independent experiments. Each assay was carried out with 6 replicates (3 duplicates) in 2 human pooled serum, 2 in culture media and 2 in standard diluent with samples containing different concentrations of CD31. 2 standard curves were run on each plate. **The overall intra-assay coefficient of variation has been calculated to be 4.0%.**

Session	Sample	Mean CD31 ng/ml	SD	CV (%)
Session 1	Sample 1	8.16	0.48	5.9
	Sample 2	2.88	0.09	3.1
	Sample 3	7.23	0.29	4.0
	Sample 4	2.05	0.14	6.6
	Sample 5	6.88	0.27	3.9
	Sample 6	1.82	0.05	2.5
Session 2	Sample 1	7.97	0.26	3.3
	Sample 2	2.74	0.06	2.2
	Sample 3	6.93	0.16	2.3
	Sample 4	2.06	0.24	11.6
	Sample 5	6.61	0.19	2.8
	Sample 6	1.99	0.04	1.8
Session 3	Sample 1	8.58	0.31	3.6
	Sample 2	2.98	0.03	1.1
	Sample 3	7.12	0.36	5.1
	Sample 4	2.05	0.04	2.1
	Sample 5	6.63	0.46	7.0
	Sample 6	1.60	0.05	3.0



## Inter-assay

Assay to assay reproducibility within one laboratory was evaluated in three independent experiments by two technicians. Each assay was carried out with 6 replicates (3 duplicates) in 2 human pooled serum, 2 in culture media and 2 in standard diluent with samples containing different concentrations of CD31. 2 standard curves were run on each plate. **The calculated overall coefficient of variation was 5.7%.**

	<i>Sample 1</i>	<i>Sample 2</i>	<i>Sample 3</i>	<i>Sample 4</i>	<i>Sample 5</i>	<i>Sample 6</i>
<b>Mean</b> CD31 ng/ml	8.24	2.86	7.09	2.05	6.71	1.80
<b>SD</b>	0.42	0.12	0.28	0.14	0.31	0.17
<b>CV (%)</b>	<b>5.0</b>	<b>4.1</b>	<b>3.9</b>	<b>6.8</b>	<b>4.6</b>	<b>9.5</b>

## 12.4. Dilution Parallelism

Two serum samples spiked in BSA or in RPMI with different levels of CD31 and a serum were analyzed at three serial two fold dilutions (1:2 to 1:8) with two replicates each. Recoveries ranged from 91 to 123% with an overall mean recovery of 110%.

## 12.5. Spike Recovery

The spike recovery was evaluated by spiking two concentrations of CD31 in human serum and cell culture media in 3 separate experiments. Recoveries ranged from 85 to 120% with an overall mean recovery of 105% in serum and ranged from 103 to 132% with an overall mean recovery of 118% in RPMI.

## 12.6. Expected serum values

A panel of 20 human sera and 20 plasma samples were tested for CD31. See results below:

Sample Matrix	Number of samples evaluated	Range (ng/ml)	Mean (ng/ml)	Standard deviation (ng/ml)
Serum	20	9.0-23.7	15.0	3.3
Plasma	20	7.5-18.1	14.0	2.7

## 13. ASSAY SUMMARY

**Total procedure length: 1 hour, 45 min**

**Add 100 µl of sample, control and diluted standard  
and 50 µl Biotinylated anti-CD31**



**Incubate 1 hour at room temperature**




**Wash three times**



**Cell Sciences, Inc.®**  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888-769-1246  
Phone: 978-572-1070  
Fax: 978-992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)

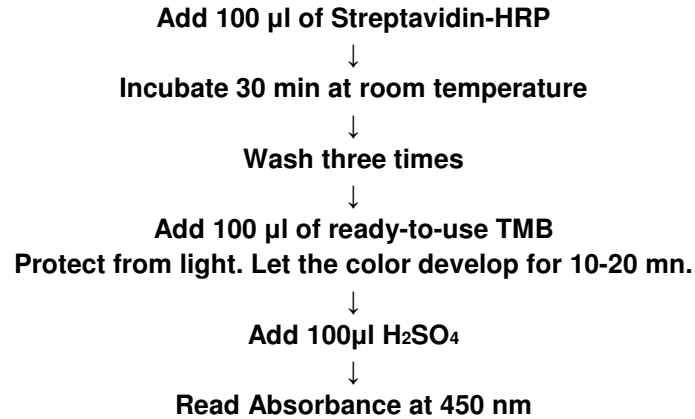

**NOT FOR HUMAN USE. FOR RESEARCH ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.**



**Cell Sciences, Inc.**<sup>®</sup>  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888-769-1246  
Phone: 978-572-1070  
Fax: 978-992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)